

Arbitrary Function Generator

AFG-3021, AFG-3022, AFG-3031 & AFG-3032

QUICK START GUIDE

GW INSTEK PART NO. 82FG-3032oMC1



ISO-9001 CERTIFIED MANUFACTURER

GW INSTEK

March 2016 edition

This manual contains proprietary information, which is protected by copyright. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Good Will Corporation.

The information in this manual was correct at the time of printing. However, Good Will continues to improve its products and therefore reserves the right to change the specifications, equipment, and maintenance procedures at any time without notice.

Good Will Instrument Co., Ltd.
No. 7-1, Jhongsing Rd., Tucheng City, Taipei County 236, Taiwan.

Table of Contents

| | |
|---|----|
| SAFETY INSTRUCTIONS | 4 |
| GETTING STARTED | 10 |
| Main Features | 10 |
| Panel Overview..... | 12 |
| Selecting a Waveform | 20 |
| Modulation..... | 23 |
| Sweep..... | 26 |
| Burst | 26 |
| ARB | 27 |
| Utility Menu | 30 |
| AFG-3021, AFG-3022, AFG-3031 & AFG-3032 Specifications | 33 |
| Declaration of Conformity | 40 |

S SAFETY INSTRUCTIONS

This chapter contains important safety instructions that should be followed when operating and storing the function generator. Read the following before any operation to ensure your safety and to keep the function generator in the best condition.

Safety Symbols

These safety symbols may appear in this manual or on the instrument.



Warning: Identifies conditions or practices that could result in injury or loss of life.



Caution: Identifies conditions or practices that could result in damage to the function generator or to other objects or property.



DANGER High Voltage



Attention: Refer to the Manual



Signal ground. Chassis ground



Signal ground. Isolated from other channels and ground.



Do not dispose electronic equipment as unsorted municipal waste. Please use a separate collection facility or contact the supplier from which this instrument was purchased.

Safety Guidelines

General Guideline



CAUTION

- Do not place heavy objects on the instrument.
- Do not place flammable objects on the instrument.
- Avoid severe impact or rough handling that may damage the function generator.
- Avoid discharges of static electricity on or near the function generator.
- Use only mating connectors, not bare wires, for the terminals.
- The instrument should only be disassembled by a qualified technician.
- Do not apply more than 42Vpk to any input/output ground or to the chassis ground.
- Do not apply voltage to the output terminals to avoid damage to the instrument.
- Do not apply more than $\pm 5V$ to the trigger or MOD input terminals to avoid damage to the instrument.

(Measurement categories) EN 61010-1:2010 specifies the measurement categories and their requirements as follows. The AFG-30XX falls under category II.

- Measurement category IV is for measurement performed at the source of a low-voltage installation.
- Measurement category III is for measurement performed in a building installation.
- Measurement category II is for measurement performed on circuits directly connected to a low voltage installation.
- Measurement category I is for measurements performed on circuits not directly connected to Mains.

-
- | | |
|---|---|
| Power Supply | <ul style="list-style-type: none">• AC Input voltage: 100 - 240V AC, 50 - 60Hz. |
|  WARNING | <ul style="list-style-type: none">• Connect the protective grounding conductor of the AC power cord to an earth ground to prevent electric shock. |
-
- | | |
|---|--|
| Fuse | <ul style="list-style-type: none">• Fuse type: AFG-3032&3022: T1A/250V AFG-3021&3031: T0.63A/250V |
|  WARNING | <ul style="list-style-type: none">• Only qualified technicians should replace the fuse.• To ensure fire protection, replace the fuse only with the specified type and rating.• Disconnect the power cord and all test leads before replacing the fuse.• Make sure the cause of the fuse blowout is fixed before replacing the fuse. |
-
- | | |
|---|--|
| Ground | <ul style="list-style-type: none">• The AFG-30XX is a floating function generator; the AFG-30XXs' common ground is electrically isolated from the chassis ground by a 42Vpk isolation voltage (DC + peak AC). Exceeding 42Vpp may cause damage to the internal circuits. |
|  CAUTION | <ul style="list-style-type: none">• Do not short the chassis ground with CH1(MAIN)'s or CH2's common ground if there is a potential voltage difference between them. Doing so may damage the unit or externally connected equipment.• If there is a potential voltage between CH1's and CH2's common ground, do not short them. Doing so may damage the unit or externally connected equipment. |
-
- | | |
|---|--|
|  WARNING | <ul style="list-style-type: none">• To avoid electric shock ensure that the output voltage and floating voltage does not exceed 42Vpk in total.• Do not touch any exposed connectors when the unit is being operated. |
|---|--|
-

- Cleaning the function generator
- Disconnect the power cord before cleaning the function generator.
 - Use a soft cloth dampened in a solution of mild detergent and water. Do not spray any liquid into the function generator.
 - Do not use chemicals containing harsh products such as benzene, toluene, xylene, and acetone.
-

- Operation Environment
- Location: Indoor, no direct sunlight, dust free, almost non-conductive pollution (Note below) and avoid strong magnetic fields.
 - Relative Humidity: < 80%
 - Altitude: < 2000m
 - Temperature: 0°C to 40°C
- (Pollution Degree) EN 61010-1:2010 specifies pollution degrees and their requirements as follows. The function generator falls under degree 2.
- Pollution refers to “addition of foreign matter, solid, liquid, or gaseous (ionized gases), that may produce a reduction of dielectric strength or surface resistivity”.
- Pollution degree 1: No pollution or only dry, non-conductive pollution occurs. The pollution has no influence.
 - Pollution degree 2: Normally only non-conductive pollution occurs. Occasionally, however, a temporary conductivity caused by condensation must be expected.
 - Pollution degree 3: Conductive pollution occurs, or dry, non-conductive pollution occurs which becomes conductive due to condensation which is expected. In such conditions, equipment is normally protected against exposure to direct sunlight, precipitation, and full wind pressure, but neither temperature nor humidity is controlled.
-

- Storage environment
- Location: Indoor
 - Relative Humidity: < 70%
 - Temperature: -10°C to 70°C
-

Disposal

Do not dispose this instrument as unsorted municipal waste. Please use a separate collection facility or contact the supplier from which this instrument was purchased. Please make sure discarded electrical waste is properly recycled to reduce environmental impact.

Class A Device**WARNING**

The AFG-30XX function generators are categorized as Class A equipment. Class A equipment is intended for use in an industrial environment. Class A equipment may have potential difficulties in ensuring electromagnetic compatibility in other environments, due to conducted as well as radiated disturbances.

Power cord for the United Kingdom

When using the function generator in the United Kingdom, make sure the power cord meets the following safety instructions.

NOTE: This lead/appliance must only be wired by competent persons

 **WARNING: THIS APPLIANCE MUST BE EARTHED**

IMPORTANT: The wires in this lead are coloured in accordance with the following code:

| | |
|----------------|--------------|
| Green/ Yellow: | Earth |
| Blue: | Neutral |
| Brown: | Live (Phase) |



As the colours of the wires in main leads may not correspond with the coloured marking identified in your plug/appliance, proceed as follows:

The wire which is coloured Green & Yellow must be connected to the Earth terminal marked with either the letter E, the earth symbol \oplus or coloured Green/Green & Yellow.

The wire which is coloured Blue must be connected to the terminal which is marked with the letter N or coloured Blue or Black.

The wire which is coloured Brown must be connected to the terminal marked with the letter L or P or coloured Brown or Red.

If in doubt, consult the instructions provided with the equipment or contact the supplier.

This cable/appliance should be protected by a suitably rated and approved HBC mains fuse: refer to the rating information on the equipment and/or user instructions for details. As a guide, a cable of 0.75mm² should be protected by a 3A or 5A fuse. Larger conductors would normally require 13A types, depending on the connection method used.

Any exposed wiring from a cable, plug or connection that is engaged in a live socket is extremely hazardous. If a cable or plug is deemed hazardous, turn off the mains power and remove the cable, any fuses and fuse assemblies. All hazardous wiring must be immediately destroyed and replaced in accordance to the above standard.

GETTING STARTED

The Getting started chapter introduces the function generator's main features, appearance, set up procedure and power-up.

Note: Throughout this document, "AFG-30XX" refers to the AFG-3021, AFG-3022, AFG-3031 & AFG-3032, unless stated otherwise.

Main Features

| Model name | Frequency bandwidth | Channels |
|------------|---------------------|---|
| AFG-3021 | 20MHz | 1 (signal ground chassis isolation) |
| AFG-3022 | 20MHz | 2 (signal ground chassis isolation and channel isolation) |
| AFG-3031 | 30MHz | 1 (signal ground chassis isolation) |
| AFG-3032 | 30MHz | 2 (signal ground chassis isolation and channel isolation) |


- Performance
- DDS Function Generator series
 - 1 μ Hz high frequency resolution maintained at full range
 - 1ppm frequency stability
 - Full Function Arbitrary Waveform Capability
 - 250 MSa/s sample rate
 - 125 MSa/s repetition rate
 - 8 M-point waveform length
 - 16-bit amplitude resolution

| | |
|-----------|--|
| | <ul style="list-style-type: none">-Ten 8 M waveform memories-True waveform output to display-D W R (Direct Waveform Reconstruction) capability-Waveform editing capability sans PC-N Cycle and Infinite output mode selectable• -60dBc low distortion sine wave |
| Features | <ul style="list-style-type: none">• Sine, Square, Triangle, Pulse, Ramp, Noise, DC standard waveforms• Int/Ext AM, FM, PWM, FSK, PM, SUM modulation• Modulation/sweep signal output• Burst function with internal and external triggers• Store/recall 10 groups of setting memories• Output overload protection• Two channel tracking (AFG-3022/3032 only)• 42Vpk signal ground chassis isolation and 42Vpk channel isolation• Multi-unit synchronized control• DSO Link function to transfer captured waveforms from the DSO to the function generator• Harmonic waveform function• Pulse waveform with configurable rise times & fall times• Frequency and amplitude sweep |
| Interface | <ul style="list-style-type: none">• Interface: LAN, USB (standard), GPIB (optional)• 4.3 inch color TFT LCD (480 × 272) Graphical User Interface• AWES (Arbitrary Waveform Editing Software) PC software |


Panel Overview

Front Panel

AFG-3021/3031

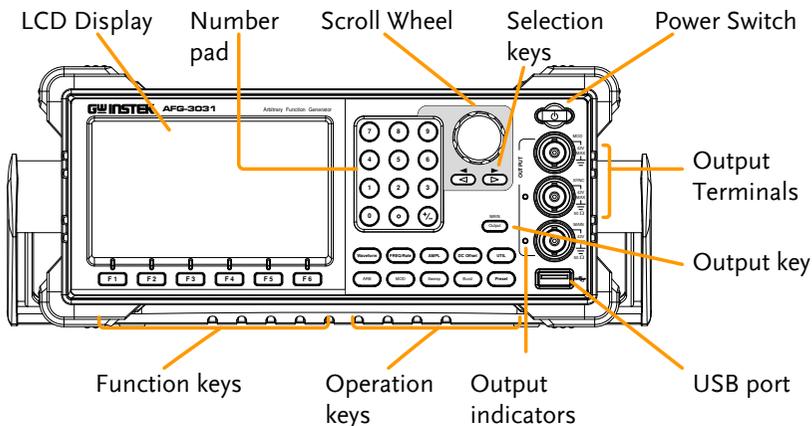


AFG-3022/3032

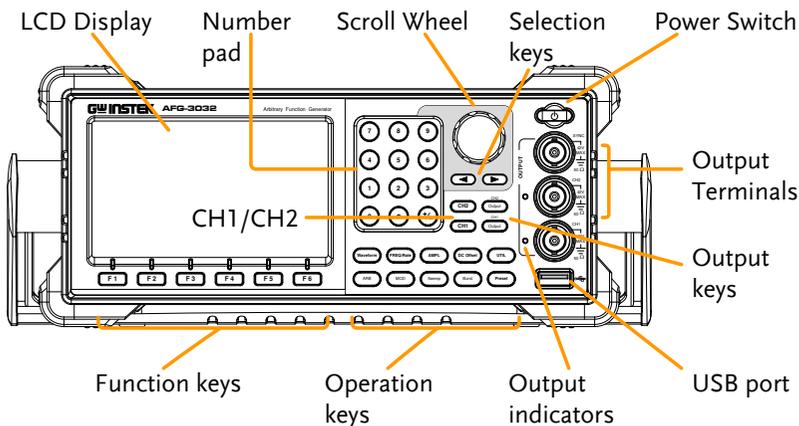

LCD display TFT color LCD display, 480 x 272 resolution.


Function keys:
F1~F6  Activates the functions which appear in the bottom of the LCD display.

Operation keys

 Waveform is used to select a waveform type.

 The FREQ/Rate key is used to set the frequency or sample rate.


 AMPL sets the waveform amplitude.

 Sets the DC offset.

 The UTIL key is used to access the save and recall options, set the remote interface (USB, GPIB, LAN), use DSO link (AFG-3021/3031), update and view the firmware version, access the calibration options, output impedance settings (AFG-3021/3031 only), set the language and access the help menu.

 ARB is used to set the arbitrary waveform parameters.

 The MOD, Sweep and Burst keys are used to set the modulation, sweep and burst settings and parameters.







Preset  The preset key is used to recall a preset state.

| | | |
|--------------------------------|---|---|
| Main Output (AFG-3021/3031) |  | The Output key is used to turn on or off the waveform output. |
|--------------------------------|---|---|


| | | |
|--------------------------------------|---|---|
| CH1/CH2 Output (AFG-3022/3032) |  | CH1/CH2 Output key. These keys are used to turn the output on or off for each individual channel. |
|--------------------------------------|---|---|

| | | |
|----------------------------|--|--|
| CH1/CH2 (AFG-3022/3032) |   | The CH1/CH2 keys are used to access the DSO link function, output impedance settings and phase settings for the AFG-3022 & AFG-3032. |
|----------------------------|--|--|
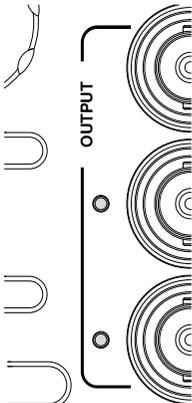
| | | |
|-------------------|---|--|
| Output indicators |  | When an Output indicator is green, it indicates that the output is active. |
|-------------------|---|--|

| | | |
|--------------------|--|---|
| USB host connector |  | The USB Host connector is used to save and restore data as well as update the firmware. |
|--------------------|--|---|

Output terminals
(AFG-3021/3031)



Modulation output terminal for the AM, FM, PWM, PM, SUM or sweep function.



The SYNC output terminal outputs a TTL logic level signal in phase with the zero phase position of the main output. 50Ω output impedance.




The primary output terminal. 50Ω output impedance.

Note: The MAIN ground has a common ground with the MOD output, SYNC and MOD input terminals. They are also isolated from the chassis ground and the 10MHz REF IN ground by an isolation voltage of 42Vpk.

Output terminals
(AFG-3022/3032)



The SYNC output terminal outputs a TTL logic level signal in phase with the zero phase position of the CH1 output. 50Ω output impedance.



CH2 output terminal. 50Ω output impedance.




CH1 output terminal. 50Ω output impedance.

Note: The CH1, CH2 and 10MHz REF IN ground are isolated from each other and from the chassis ground by an isolation voltage of 42Vpk.

The CH1 ground has a common ground with the MOD output, SYNC and the CH1 MOD input terminals.

The CH2 ground has a common ground with the CH2 MOD input terminal.

Standby key




The standby key is used to turn the function generator on (green) or to put the function generator into standby mode (red).

Selection keys




Used to select digits when editing parameters.

Scroll Wheel




The scroll wheel is used to edit values and parameters.



Decrease

Increase


Keypad




The digital keypad is used to enter values and parameters. The keypad is often used in conjunction with the selection keys and variable knob.

Rear Panel


AFG-3021/3031

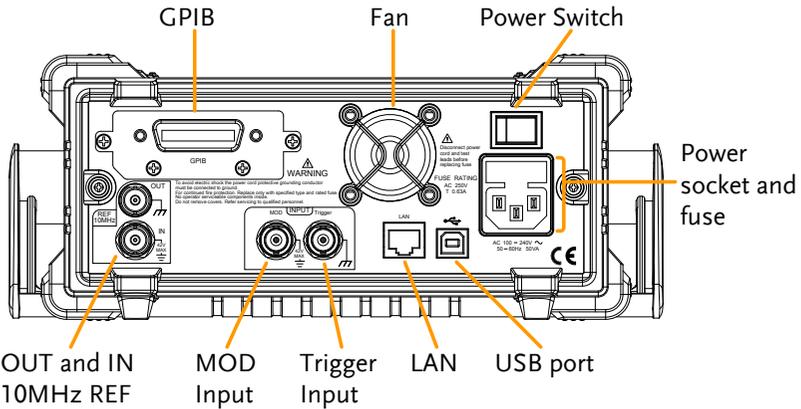

AFG-3022/3032

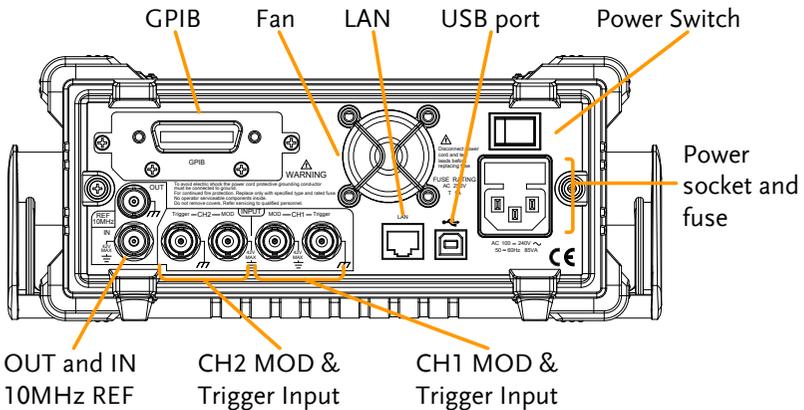

10MHz REF OUT




10 MHz reference output.

10MHz REF IN


10 MHz reference input. The 10MHz REF IN ground has a 42Vpk isolation from the CH1(MAIN), CH2 and chassis ground.

Trigger Input



External trigger input. Used to receive external trigger signals. For the AFG-3022/3032 there is a separate trigger input for CH1 and CH2.

MOD input



Modulation input terminal. For the AFG-3022/3032 there is a separate modulation input for CH1 and CH2.


Note: The CH1/CH2 MOD input ground are isolated from each other and from the chassis ground by an isolation voltage of 42Vpk.

The CH1 MOD input shares ground with the CH1 ground.

The CH2 MOD input shares ground with the CH2 ground.

Fan

Power Socket Input and fuse



Power input: 100-240V AC, 50-60Hz.

Fuse:
AFG-3032 & AFG-3022: T1A/250V
AFG-3021 & AFG-3031: T0.63A/250V

Power Switch



Main power switch.

USB B port



The USB B connector is used to connect the function generator to a PC for remote control.

LAN port




Ethernet port used for remote control (RJ45 connector).

GPIB



24 pin female GPIB connector for PC remote control.

Display

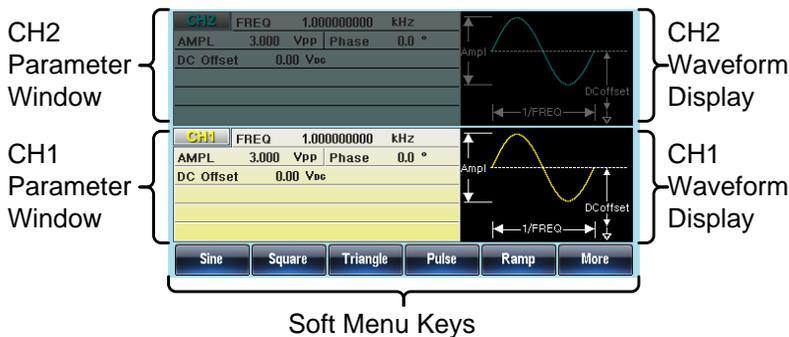

Parameter Windows These windows are used to edit the parameter values for CH1 and CH2.

Waveform Display The Waveform Display is used give an indication of the expected waveform output for each channel.


Soft Menu Keys The function keys (F1~F6) below the Soft Menu keys correspond to the soft keys.

Selecting a Waveform

Square Wave

Example: Square wave, 3Vpp, 75% duty, 1 kHz

Output




1. Press **Waveform > Square (F2)**.
2. Press **Duty(F1) > 75 > % (F5)**.
3. Press **FREQ/Rate > 1 > kHz (F5)**.
4. Press **AMPL > 3 > VPP (F6)**.
5. Press **Output**.

Input: N/A

Triangle Wave

Example: Triangle wave, 5Vpp, 10kHz

Output




1. Press **Waveform > Triangle (F3)**.
2. Press **FREQ/Rate key > 10 > kHz (F5)**.
3. Press **AMPL > 5 > VPP (F6)**.
4. Press **Output**.

Input: N/A

Sine Wave

Example: Sine wave, 10Vpp, 100kHz

Output




1. Press **Waveform > Sine (F1)**.
2. Press **FREQ/Rate > 100 > kHz (F5)**.
3. Press **AMPL > 10 > VPP (F6)**.
4. Press **Output**.

Input: N/A

Pulse Wave

Example: Pulse wave, 10Vpp, 100kHz, 5us pulse width

Output




Input: N/A

1. Press **FREQ/Rate** > 100 > kHz (F5).
2. Press **Waveform** > Pulse (F4).
3. Press **Width** (F1) > 5 > uSEC (F3).
4. Press **AMPL** > 10 > VPP (F6).
5. Press **Output**.

Noise Wave

Example: White noise output

Output




Input: N/A

1. Press **Waveform** > More (F6) > Noise (F1).
2. Press **Output**.

Harmonic Wave

Example: 10kHz harmonic sine wave, odd & even (all) harmonics, up to the 3rd order (2nd(5Vpp), 3rd(2Vpp), 0° phase).

Output



Input: N/A

1. Press **Waveform** > More (F6) > Harmonic (F2).
2. Press **Total** (F1) > 3 > Enter (F1).
3. Press **Type** (F2) > ALL (F3).
4. Press **Order** (F3).
5. Press **Order** (F1) > 2 > Enter (F1).
6. Press **Amp**(F2) > 5 > VPP (F2).
7. Press **Phase**(F3) > 0 > Degree (F1).


8. Press **Order (F1) > 3 > Enter (F1)**.
9. Press **Amp(F2) > 2 > VPP (F2)**.
10. Press **Phase(F3) > 0 > Degree (F1)**.
11. Press **Output**.

Modulation

AM

Example: AM modulation. 100Hz modulating square wave. 1kHz Sine wave carrier. 80% modulation depth.

Output




Input: N/A

1. Press **MOD > AM (F1)**.
2. Press **Waveform > Sine (F1)**.
3. Press **Freq/Rate > 1 > kHz (F5)**.
4. Press **MOD > AM (F1) > Shape (F4) > Square (F2)**.
5. Press **MOD > AM (F1) > AM Freq (F3)**.
6. Press **100 > Hz (F2)**.
7. Press **MOD > AM (F1) > Depth (F2)**.
8. Press **80 > % (F1)**.
9. Press **MOD > AM (F1) > Source (F1) > INT (F1)**.
10. Press **Output**.

FM

Example: FM modulation. 100Hz modulating square wave. 1kHz sine wave carrier. 100 Hz frequency deviation. Internal source.

Output



Input: N/A


1. Press **MOD > FM (F2)**.
2. Press **Waveform > Sine (F1)**.
3. Press **Freq/Rate > 1 > kHz (F5)**.
4. Press **MOD > FM (F2) > Shape (F4) > Square (F2)**.
5. Press **MOD > FM (F2) > FM Freq (F3)**.
6. Press **100 > Hz (F2)**.
7. Press **MOD > FM (F2) > Freq Dev (F2)**.
8. Press **100 > Hz (F3)**.

9. Press **MOD > FM (F2) > Source (F1) > INT (F1)**.
10. Press **Output**.

FSK Modulation

Example: FSK modulation. 100Hz hop frequency. 1kHz carrier wave. Triangle wave. 10 Hz rate. Internal source.

Output




Input: N/A

1. Press **MOD > FSK (F3)**.
2. Press **Waveform > Triangle (F3)**.
3. Press **Freq/Rate > 1 + kHz (F5)**.
4. Press **MOD > FSK (F3) > FSK Rate (F3)**.
5. Press **10 > Hz (F2)**.
6. Press **MOD > FSK (F3) > Hop Freq (F2)**.
7. Press **100 > Hz (F3)**.
8. Press **MOD > FSK (F3) > Source (F1) > INT (F1)**.
9. Press **Output**.

PM

Example: PM modulation. 100Hz phase frequency. Sine wave shape. 180° phase deviation. 1kHz sine wave carrier.

Output




Input: N/A

1. Press **MOD > PM (F4)**.
2. Press **Waveform > Sine (F1)**.
3. Press **Freq/Rate > 1 > kHz (F5)**.
4. Press **MOD > PM (F4) > Shape (F4) > Sine (F1)**.
5. Press **MOD > PM (F4) > PM Freq (F3)**.
6. Press **100 > Hz (F2)**.
7. Press **MOD > PM (F2) > Phase Dev (F2)**.
8. Press **180 > Degree (F1)**.

SUM Modulation

Example: FSK modulation. 100Hz SUM frequency. 50% SUM amplitude. 1kHz carrier sine wave. Triangle wave shape. Internal source.

Output




Input: N/A

1. Press **MOD > SUM (F5)**.
2. Press **Waveform > Sine (F1)**.
3. Press **Freq/Rate > 1 + kHz (F5)**.
4. Press **MOD > SUM (F5) > SUM Freq (F3)**.
5. Press **100 > Hz (F2)**.
6. Press **MOD > SUM (F5) > SUM Ampl (F2)**.
7. Press **50 > % (F1)**.
8. Press **MOD > SUM (F5) > Shape (F4) > Triangle (F3)**
9. Press **MOD > SUM (F5) > Source (F1) > INT (F1)**.
10. Press **Output**.

PWM Modulation

Example: PWM modulation. 800Hz carrier wave. 15 kHz modulating sine wave. 50% duty cycle. Internal source.

Output




Input: N/A

1. Press **Waveform > Square (F2)**.
2. Press **MOD > PWM (F4)**.
3. Press **FREQ/Rate key > 800 > Hz (F4)**.
4. Press **MOD > PWM (F4) > Shape (F4) > Sine (F1)**.
5. Press **MOD > PWM (F4) > PWM Freq (F3)**.
6. Press **15 > kHz (F3)**.
7. Press **MOD > PWM (F4) > Duty (F2)**.
8. Press **50 > % (F1)**.
9. Press **MOD > PWM (F4) > Source (F1) > INT (F1)**.
10. Press **Output**.

Sweep

Example: Frequency sweep. Start frequency 10mHz, stop frequency 1MHz. Log sweep, 1 second sweep, manual trigger.

Output




Input: N/A

1. Press **Sweep > Start (F3)**.
2. Press **10 > mHz (F2)**.
3. Press **Sweep > Stop (F4)**.
4. Press **1 > MHz (F5)**.
5. Press **Sweep > Type/MOD (F2) > Functions (F3) > Log (F2)**.
6. Press **Sweep > SWP Time (F5)**.
7. Press **1 > SEC (F2)**.
8. Press **Sweep > TRIG Type (F6) > Manual (F3)**.
9. Press **Output**.
10. Press **Trigger (F1)**.

Burst

Example: Burst mode, N-Cycle (Internally triggered), 1kHz burst frequency, burst count = 5, 10 ms burst period, 0° burst phase, internal trigger, 10 us delay.

Output



Input: N/A


1. Press **FREQ/Rate > 1 > kHz (F5)**.
2. Press **Burst > N Cycle (F1) > Cycles (F1)**.
3. Press **5 > Cyc (F5)**.
4. Press **Burst > N Cycle (F1) > Period (F4)**.
5. Press **10 > msec (F2)**.
6. Press **Burst > N Cycle (F1) > Phase (F3)**.
7. Press **0 > Degree (F5)**.
8. Press **Burst > N Cycle (F1) > TRIG Setup (F5) > INT (F1)**.
9. Press **Burst > N Cycle (F1) > TRIG Setup (F5) > Delay (F4)**.
10. Press **10 > uSEC (F2)**.
11. Press **Output**.

ARB

ARB – Add Built-In Waveform

Example: ARB Mode, exponential rise. Start 0, length 100, scale 32767.

Output




1. Press **ARB > Built in (F3) > Basic (F1) > More (F5) > Exp Rise (F1)**.
2. Press **Start (F1) > 0 > Enter (F5)**.
3. Press **Length (F2) > 100 > Enter (F5)**.
4. Press **Scale (F3), 32767 > Enter (F5) > Done (F4)**.

ARB – Add Built-In Waveform - Pulse

Example: ARB Mode, Pulse. Start 0, Frequency 1kHz, Duty 25%.

Output




1. Press **ARB > Built in (F3) > Basic (F1) > More (F5) > Pulse (F4)**.
2. Press **Frequency (F1) > 1 > kHz (F5)**.
3. Press **Duty (F2) > 25 > % (F5)**.

ARB - Add Point

Example: ARB Mode, Add point, Address 40, data 30,000.

Output




1. Press **ARB** > **Edit (F2)** > **Point (F1)** > **Address (F1)**.
2. Press **40** > **Enter (F5)**.
3. Press **Data (F2)** > **30000** > **Enter (F5)**.

ARB - Add Line

Example: ARB Mode, add line, address: data (10:30, 50:100)

Output




1. Press **ARB** > **Edit (F2)** > **Line (F2)** > **Start ADD (F1)**.
2. Press **10** > **Enter (F5)**.
3. Press **Start Data (F2)** > **30** > **Enter (F5)**.
4. Press **Stop ADD (F3)** > **50** > **Enter (F5)**.
5. Press **Stop Data (F4)** > **100** > **Enter (F5)** > **Done (F5)**.

ARB – Output Section

Example: ARB Mode, output ARB waveform, start 0, length 1000.

Output




1. Press **ARB** > **Output (F6)**.
2. Press **Start (F1)** > **0** > **Enter (F5)**.
3. Press **Length (F2)** > **1000** > **Enter (F5)**.

ARB – Output N Cycle

Example: ARB Mode, Output N Cycle, Start 0, Length 1000, N Cycle 10.

Output




1. Press **ARB > Output (F6)**.
2. Press **Start (F1) > 0 > Enter (F5)**.
3. Press **Length (F2) > 1000 > Enter (F5)**.
4. Press **N Cycle (F4)**.
5. Press **Cycles (F1) > 10 > Enter (F5)**.
6. To trigger the output once:
Press **Trigger (F5)**.

ARB – Output Infinite Cycles

Example: ARB Mode, output N cycle, start 0, length 1000, cycles infinite.

Output



1. Press **ARB > Output (F6)**.
2. Press **Start (F1) > 0 > Enter (F5)**.
3. Press **Length (F2) > 1000 > Enter (F5)**.
4. Press **Infinite (F5)**.

Utility Menu

Save

Example: Save to memory file #5.

1. Press **UTIL > Memory (F1)**.
2. Choose a file using the scroll wheel.
3. Press **Store (F1) > Done (F5)**.

Recall


Example: Recall memory file #5.

1. Press **UTIL > Memory (F1)**.
2. Choose a file using the scroll wheel.
3. Press **Recall (F2) > Done (F5)**.

Interface GPIB

Example: GPIB interface, address 10.

GPIB



1. Press **UTIL > Interface (F2) > GPIB (F1) > Address (F1)**.
2. Press **10 > Done (F5)**.

Interface LAN

Example: LAN interface, DHCP IP configuration.

LAN



1. Press **UTIL > Interface (F2) > LAN (F3)**.
2. Press **Config (F2) > DHCP (F1)**.
3. Press **Done (F3)**.

Interface USB

Example: USB interface.




1. Press **UTIL > Interface (F2) > USB (F2)**.

Dual Channel – Frequency Coupling

Example: 1kHz offset coupling. AFG-3022, 3032 only.

Output




1. Press **UTIL > Dual Ch (F5) > Freq Cpl (F1)**.
2. Press **Offset (F2) > 10 > kHz (F4)**.

Dual Channel – Amplitude Coupling

Example: Amplitude coupling. AFG-3022, 3032 only.

Output




1. Press **UTIL > Dual Ch (F5) > Ampl Cpl (F2)**.
2. Press **ON (F1)**.

Dual Channel – Tracking

Example: Inverted tracking. AFG-3022, 3032 only.

Output



1. Press **UTIL > Dual Ch (F5) > Tracking (F3)**.
2. Press **Inverted (F3)**.

AFG-3021, AFG-3022, AFG-3031 & AFG-3032 Specifications

The specifications apply when the function generator is powered on for at least 30 minutes under +20°C~+30°C.

| General Specification | | AFG-3021 | AFG-3031 | AFG-3022 | AFG-3032 |
|-----------------------|--|---|----------|----------|----------|
| Channels | | 1 | 1 | 2 | 2 |
| Instrument | | Isolated | Isolated | Isolated | Isolated |
| Chassis | | | | | |
| Signal Ground | | — | — | Isolated | Isolated |
| Waveforms | | | | | |
| Standard | | Sine, Square, Ramp, Pulse, Noise, Harmonic, DC | | | |
| Arbitrary Waveforms | | | | | |
| ARB Function | | Built in | | | |
| Sample Rate | | 250 MSa/s | | | |
| Repetition Rate | | 125MHz | | | |
| Waveform Length | | 8M points | | | |
| Amplitude Resolution | | 16 bits | | | |
| Non-Volatile Memory | | Ten 8M waveforms(1) | | | |
| User-defined | | Any section from 2 to 8M points | | | |
| Output Section | | | | | |
| Trigger | | Infinite/Manual/External | | | |
| Built-in | | Sine, Square, Ramp, Sinc, Exp Rise, Exp Fall, DC, Pulse, Abstan, Haver cosine, Sinever, | | | |
| Arbitrary | | Abssin, Haversine, Stair_down, Abs sinehalf, N_pulse, Stair_UD, Ampalt, Negramp, Stair_up, Attalt, Rectpuls1, Stepresp, Diric_even, Roundhalf, Trapezia, Diric_odd, Sawtoot, Tripuls1, Gauspuls1, Sinetra, Dlorentz, Ln, Sqrt, Since, Lorentz, Xsquare, Gauss, Arccos, Arctan, Sech, Arccot, Arctanh, Sinh, Arccsc, Cosh, Tan, Arcsec, Cot, Tanh, Arcsin, Csc, Arcsinh, Sec, Barthannwin, Chebwin, Kaiser, Bartlett, Flattopwin, Triang, Blackman, Hamming, Tukeywin, Bohmanwin, Hann | | | |

| Frequency Characteristics | | | | | |
|----------------------------|------------------|---|---|-------|-------|
| Range | Sine | 20MHz | 20MHz | 30MHz | 30MHz |
| | Square | 20MHz | 20MHz | 30MHz | 30MHz |
| | Triangle, Ramp | | 1MHz | | |
| Resolution | | | | 1μHz | |
| Accuracy | Stability | | ±1 ppm 0 to 50°C ±0.3 ppm 18 to 28°C | | |
| | Aging | | ±1 ppm, per 1 year | | |
| | Tolerance | | ≤1 μHz | | |
| Output Characteristics(2) | | | | | |
| Amplitude | Range | 1 mVpp to 10 Vpp(into 50Ω) 2 mVpp to 20 Vpp(open-circuit) | | | |
| | Accuracy | ± 1% of setting ±1 mVpp (at 1 kHz/into 50Ω without DC offset) | | | |
| | Resolution | 0.1 mV or 4 digits | | | |
| | Flatness | ±0.1dB: <10 MHz ±0.2 dB: 10 MHz to 30 MHz (sinewave relative to 1 kHz/into 50Ω) | | | |
| | Units | Vpp, Vrms, dBm, | | | |
| Offset | Range | ±5 Vpk ac +dc (into 50Ω) ±10Vpk ac +dc (open circuit) | | | |
| | Accuracy | 1% of setting + 2 mV + 0.5% Amplitude | | | |
| Waveform | Impedance | 50Ω typical (fixed) | | | |
| Output | | > 10MΩ (output disabled) | | | |
| | Protection | Short-circuit protected Overload relay automatically disables main output | | | |
| | Ground Isolation | 42Vpk max. | | | |
| | Sync Output | Level | TTL-compatible into>1kΩ | | |
| | Impedance | 50Ω nominal | | | |
| | Ground Isolation | 42Vpk max. (same ground as CH1 output) | | | |
| Sine wave Characteristics | | | | | |
| Distortion(5) | Harmonic | -60 dBc | DC ~ 1 MHz, Ampl<3 Vpp | | |
| | | -55 dBc | DC ~ 1 MHz, Ampl>3 Vpp | | |
| | | -45 dBc | 1MHz ~ 5 MHz, Ampl>3 Vpp | | |
| | | -30 dBc | 5MHz ~ 30 MHz, Ampl>3 Vpp | | |
| Total Harmonic Distortion | | < 0.2%+0.1mVrms DC to 20 kHz | | | |
| Spurious (non-harmonic)(5) | | -60 dBc | DC~1 MHz | | |
| | | -50 dBc | 1MHz~20MHz | | |
| | | -50 dBc + 6 dBc/octave 1MHz~30MHz(AFG-3031/3032 only) | | | |
| Phase Noise | | < -110dBc/Hz (typical), 15kHz offset, fc=10MHz | | | |

| Square wave Characteristics | | | | |
|-----------------------------|---|-----------------------------|-----------------------------|-----------------------------|
| Rise/Fall Time | <8 ns(3) | | | |
| Overshoot | <5% | | | |
| Asymmetry (@50% duty) | 1% of period +1 ns | | | |
| Variable Duty Cycle | 20.0% to 80.0%: ≤ 20 MHz | 20.0% to 80.0%: ≤ 25 MHz | 20.0% to 80.0%: ≤ 20 MHz | 20.0% to 80.0%: ≤ 25 MHz |
| | | 40.0% to 60.0%: 25~30MHz | | 40.0% to 60.0%: 25~30MHz |
| Jitter | 0.01%+525ps < 2 MHz 0.1%+75ps > 2 MHz | | | |
| Ramp Characteristics | | | | |
| Linearity | < 0.1% of peak output | | | |
| Variable Symmetry | 0% to 100% (0.1% resolution) | | | |
| Pulse Characteristics | | | | |
| Frequency | 1uHz ~ 20MHz | 1uHz ~ 25MHz | 1uHz ~ 20MHz | 1uHz ~ 25MHz |
| Width | 20ns ~ 999.83ks (Extended mode 0.00ns ~ 1,000ks ⁽⁶⁾) | | | |
| | Width - 0.625 * [(Rise Time - 0.6nS) + (Fall Time - 0.6nS)] ≥ 0 | | | |
| | Period ≥ Width+ 0.625 * [(Rise Time - 0.6nS)+(Fall Time - 0.6nS)] | | | |
| Duty Setting Range | 0.017% to 99.983% (Extended mode 0.0000% to 100.0000% ⁽⁶⁾) | | | |
| Period | 40ns ~ 1000000s | | | |
| Rise time and Fall Time | 9.32ns ~ 799.89ks | | | |
| Resolution | 0.0001% | | | |
| Overshoot | < 5% | | | |
| Jitter | 50ps typical (<10kHz) | | | |
| Noise | | | | |
| Noise Type | Gaussian | | | |
| Noise Bandwidth | 100MHz equivalent bandwidth | | | |
| Harmonic | | | | |
| Harmonic Order | ≤ 8 | | | |

| | | | | | |
|----------------------------------|----------------------|--|-------------|-------------|-------------|
| | Harmonic Type | Even, Odd, All, User Amplitude and Phase can be set for all harmonics | | | |
| AM Modulation | | | | | |
| | Carrier Waveforms | Sine, Square, Triangle, Ramp, Pulse, Noise, Arb | | | |
| | Modulating Waveforms | Sine, Square, Triangle, Up/Dn Ramp | | | |
| | Modulating Frequency | 2mHz to 20kHz | | | |
| | Depth | 0% to 120.0% | | | |
| | Source | Internal / External | | | |
| FM Modulation | | | | | |
| | Carrier Waveforms | Sine, Square, Triangle, Ramp | | | |
| | Modulating Waveforms | Sine, Square, Triangle, Up/Dn Ramp | | | |
| | Modulating Frequency | 2mHz to 20kHz | | | |
| | Peak Deviation | DC to 30MHz(1 uHz resolution) (DC to 20MHz for AFG-3021/3022) | | | |
| | Source | Internal / External | | | |
| PWM | | | | | |
| | Carrier Waveforms | Square | | | |
| | Modulating Waveforms | Sine, Square, Triangle, Up/Dn Ramp | | | |
| | Modulating Frequency | 2mHz to 20kHz | | | |
| | Deviation | 0% ~ 100.0% of pulse width, 0.1% resolution | | | |
| | Source | Internal / External | | | |
| FSK | | | | | |
| | Carrier Waveforms | Sine, Square, Triangle, Ramp | | | |
| | Modulating Waveforms | 50% duty cycle square | | | |
| | Internal Rate | 2mHz to 1MHz | | | |
| | Frequency Range | DC to 20MHz | DC to 30MHz | DC to 20MHz | DC to 30MHz |
| | Source | Internal / External | | | |
| Additive modulation (Sum) | | | | | |
| | Carrier Waveforms | Sine, Triangle, Ramp, Pulse, Noise | | | |
| | Modulating Waveforms | Sine, Square, Triangle, Up/Dn Ramp | | | |

| | | |
|----------------------------------|-------------------------------|---|
| | Ratio | 0% to 100% of carrier amplitude, 0.01% resolution |
| | Modulating Frequency | 2mHz to 20kHz |
| | Source | Internal /External |
| PM | Carrier Waveforms | Sine, Triangle, Ramp |
| | Modulating Waveforms | Sine, Square, Triangle, Up/Dn Ramp |
| | Phase Deviation Setting Range | 0° to 360°, 0.1° resolution |
| | Modulating Frequency | 2mHz to 20kHz |
| | Source | Internal |
| Sweep | Waveforms | Frequency Sweep: Sine, Square, Triangle, Ramp Amplitude Sweep: Sine, Square, Triangle, Ramp, Pulse, Noise, ARB |
| | Type | Frequency, Amplitude |
| | Functions | Linear or Logarithmic |
| | Directions | Up or Down |
| | Start/Stop Frequency | Any frequency within the waveform's range |
| | Sweep Time | 1ms to 500s (1ms resolution) |
| | Trigger Mode | Single, External, Internal |
| | Trigger Source | Internal/External |
| Burst | Waveforms | Sine, Square, Triangle, Ramp, Pulse and Noise |
| | Frequency | 1μHz to 20MHz 1μHz to 30MHz(4) 1μHz to 20MHz 1μHz to 30MHz(4) |
| | Burst Count | 1 to 1000000 cycles or Infinite |
| | Start/Stop Phase | -360.0° to +360.0° (0.1° resolution) |
| | Internal Period | 1us to 500s |
| | Gate Source | External Trigger (pulse waveforms can only be used in gate mode) |
| | Trigger Source | Single, External or Internal Rate |
| | Trigger Delay | N-Cycle, Infinite: 0us to 100s(1us resolution) |
| External Modulation Input | Type | AM, FM, PWM, Sum |
| | Voltage Range | ± 5V full scale |
| | Input Impedance | 10kΩ |
| | Frequency | DC to 20kHz |

| | | |
|--|-----------------------------------|---|
| | Ground Isolation | 42Vpk max. (same ground as corresponding channel) |
| Modulation Output (AFG-3021/3031) | | |
| | Type | AM, FM, PWM, PM, Sum, Sweep |
| | Amplitude | ≥ 1Vpp |
| | Impedance | >10kΩ typical |
| External Trigger Input | | |
| | Type | For FSK, Burst, Sweep, N Cycle ARB |
| | Input Level | TTL Compatibility |
| | Slope | Rising or Falling (Selectable) |
| | Pulse Width | >100ns |
| | Input rate | DC to 1MHz |
| | Input Impedance | 10kΩ, DC coupled |
| Latency | | |
| | Sweep | <1us (typical) |
| | Burst | <0.55us (typical) |
| | ARB | < (27.5/sample rate) + 274ns |
| Jitter | | |
| | Sweep | 2.5 us |
| | Burst | 1 ns; except pulse, 300 ps |
| 10 MHz Reference Output | | |
| | Output Voltage | 1 Vp-p/50Ω square wave |
| | Output Impedance | 50Ω, AC coupled |
| | Output Frequency | 10MHz |
| 10 MHz Reference Input | | |
| | Input Voltage | 0.5Vp-p to 5Vp-p |
| | Input Impedance | 1kΩ, unbalanced, AC coupled |
| | Max. Allowed Input | ± 10Vdc |
| | Input Frequency | 10MHz ± 10Hz |
| | Waveform | Sine or square (50±5% duty) |
| | Ground Isolation | 42Vpk max. |
| External-Sync | | |
| | Phase Delay (max.) | Series Connection: $39+(N-2)*39 \pm 25nS$ Parallel connection: $(N-1)*6 \pm 25nS$ (where N=number of connected units) |
| | Maximum number of connected units | Series Connection: 4 Parallel Connection: 6 |
| | Applicable Functions | Sine, Square, Triangle, Pulse, Ramp, Harmonic, MOD, Sweep, Burst |

| | |
|--------------|---------------------------------------|
| Store/Recall | 10 Groups of Setting Memories |
| Interface | GPIB(optional), LAN, USB |
| Display | 4.3 inch TFT LCD, 480 × 3 (RGB) × 272 |

General Specifications

| | | |
|------------|-----------------------|--|
| | Power Source | AC100 - 240V, 50 - 60Hz |
| | Power | 85 VA for AFG-3032 & AFG-3022 |
| | Consumption | 50VA for AFG-3021 & AFG-3031 |
| | Operating Environment | Temperature to satisfy the specification: 18 ~ 28°C Operating temperature: 0 ~ 40°C Relative Humidity: ≤ 80%, 0 ~ 40°C ≤ 70%, 35 ~ 40°C Installation category: CAT II |
| | Operating Altitude | 2000 meters |
| | Pollution Degree | EN 61010 Degree 2, Indoor Use |
| | Storage Temperature | -10~70°C, Humidity: ≤70% |
| Dimensions | Bench Top | 265(W) x 107(H) x 374(D) |
| | Weight | Approx. 3.5kg |
| | Safety Designed to | EN 61010-1 |
| | EMC Tested to | EN 61326, EN 55011 |
| | Accessories | Test cable(GTL-110x1 for AFG-3021/3031, GTL-110x2 for AFG-3022/3032), User Manual Compact Disk × 1, Quick Start Guide × 1, Power cord × 1 |

- (1). A total of ten waveforms can be stored. (Every waveform can be composed of 8M points maximum.)
- (2). Add 1/10th of output amplitude and offset specification per °C for operation outside of 0°C to 28°C range (1-year specification).
- (3). Edge time decreased at higher frequency.
- (4). Sine and square waveforms above 25 MHz are allowed only with an “Infinite” burst count.
- (5). Harmonic distortion and Spurious noise at low amplitudes is limited by a -70 dBm floor.
- (6). Loss may occur if the pulse width is beyond the setting range of the normal mode. The pulse may vanish at times.

Declaration of Conformity

We

GOOD WILL INSTRUMENT CO., LTD.

declare that the below mentioned product

Type of Product: Arbitrary Function Generator

Model Number: AFG-3021, AFG-3031, AFG-3022, AFG-3032

are herewith confirmed to comply with the requirements set out in the Council Directive on the Approximation of the Law of Member States relating to Electromagnetic Compatibility (2014/30/EU) and Low Voltage Equipment Directive (2014/35/EU).

For the evaluation regarding the Electromagnetic Compatibility and Low Voltage Directive, the following standards were applied:

| © EMC | |
|---|--|
| EN 61326-1 : EN 61326-2-1: | Electrical equipment for measurement, control and laboratory use — EMC requirements (2013) |
| Conducted and Radiated Emissions EN 55011:2009+A1:2010 | Electrical Fast Transients EN 61000-4-4:2012 |
| Current Harmonic EN 61000-3-2:2014 | Surge Immunity EN 61000-4-5: 2006 |
| Voltage Fluctuation EN 61000-3-3:2013 | Conducted Susceptibility EN 61000-4-6: 2014 |
| Electrostatic Discharge EN 61000-4-2: 2009 | Power Frequency Magnetic Field EN 61000-4-8:2010 |
| Radiated Immunity EN 61000-4-3:2006+A1:2008+A2:2010 | Voltage Dips/ Interrupts EN 61000-4-11: 2004 |
| Low Voltage Equipment Directive 2014/35/EU | |
| Safety Requirements | EN 61010-1:2010 (Third Edition) EN 61010-2-030:2010 (First Edition) |

GOODWILL INSTRUMENT CO., LTD.

No. 7-1, Jhongsing Road, Tucheng District, New Taipei City 236, Taiwan

Tel: [+886-2-2268-0389](tel:+886-2-2268-0389)

Fax: [+886-2-2268-0639](tel:+886-2-2268-0639)

Web: <http://www.gwinstek.com>

Email: marketing@goodwill.com.tw

GOODWILL INSTRUMENT (SUZHOU) CO., LTD.

No. 521, Zhujiang Road, Snd, Suzhou Jiangsu 215011, China

Tel: [+86-512-6661-7177](tel:+86-512-6661-7177)

Fax: [+86-512-6661-7277](tel:+86-512-6661-7277)

Web: <http://www.instek.com.cn>

Email: marketing@instek.com.cn

GOODWILL INSTRUMENT EURO B.V.

De Run 5427A, 5504DG Veldhoven, The Netherlands

Tel: [+31-\(0\)40-2557790](tel:+31-(0)40-2557790)

Fax: [+31-\(0\)40-2541194](tel:+31-(0)40-2541194)

Email: sales@gw-instek.eu